



UNIVERSITY
OF WOLLONGONG
AUSTRALIA

University of Wollongong Research Online

Faculty of Science, Medicine and Health - Papers

Faculty of Science, Medicine and Health

2013

Bio-ink for on-demand printing of living cells

Cameron J. Ferris

University of Wollongong, cjf146@uowmail.edu.au

Kerry J. Gilmore

University of Wollongong, kerryg@uow.edu.au

Stephen Beirne

University of Wollongong, sbeirne@uow.edu.au

Donald McCallum

University of Wollongong, donmc@uow.edu.au

Gordon G. Wallace

University of Wollongong, gwallace@uow.edu.au

See next page for additional authors

Publication Details

Ferris, C. J., Gilmore, K. J., Beirne, S., McCallum, D., Wallace, G. G. & in het Panhuis, M. (2013). Bio-ink for on-demand printing of living cells. *Biomaterials Science*, 1 (2), 224-230.

Research Online is the open access institutional repository for the University of Wollongong. For further information contact the UOW Library:
research-pubs@uow.edu.au

Bio-ink for on-demand printing of living cells

Abstract

Drop-on-demand bioprinting allows the controlled placement of living cells, and will benefit research in the fields of tissue engineering, drug screening and toxicology. We show that a bio-ink based on a novel microgel suspension in a surfactant-containing tissue culture medium can be used to reproducibly print several different cell types, from two different commercially available drop-on-demand printing systems, over long printing periods. The bio-ink maintains a stable cell suspension, preventing the settling and aggregation of cells that usually impedes cell printing, whilst meeting the stringent fluid property requirements needed to enable printing even from many-nozzle commercial inkjet print heads. This innovation in printing technology may pave the way for the biofabrication of multi-cellular structures and functional tissue.

Keywords

ink, bio, demand, cells, printing, living

Disciplines

Medicine and Health Sciences | Social and Behavioral Sciences

Publication Details

Ferris, C. J., Gilmore, K. J., Beirne, S., McCallum, D., Wallace, G. G. & in het Panhuis, M. (2013). Bio-ink for on-demand printing of living cells. *Biomaterials Science*, 1 (2), 224-230.

Authors

Cameron J. Ferris, Kerry J. Gilmore, Stephen Beirne, Donald McCallum, Gordon G. Wallace, and Marc in het Panhuis

Bio-ink for on-demand printing of living cells

Cameron J. Ferris,^{a,b}, Kerry J. Gilmore,^a Stephen Beirne,^a Donald McCallum,^{a,b} Gordon G. Wallace^{a,*} and Marc in het Panhuis^{a,b,*}

Received (in XXX, XXX) Xth XXXXXXXXXX 20XX, Accepted Xth XXXXXXXXXX 20XX

DOI: 10.1039/b000000x

Drop-on-demand bioprinting allows the controlled placement of living cells, and will benefit research in the fields of tissue engineering, drug screening and toxicology. We show that a bio-ink based on a novel microgel suspension in surfactant-containing tissue culture medium can be used to reproducibly print several different cell types, from two different commercially available drop-on-demand printing systems, over long printing periods. The bio-ink maintains a stable cell suspension, preventing the settling and aggregation of cells that usually impedes cell printing, whilst meeting the stringent fluid property requirements needed to enable printing even from many-nozzle commercial inkjet print heads. This innovation in printing technology may pave the way to the biofabrication of multi-cellular structures and functional tissue.

Introduction

Bioprinting is an emerging technology that highlights a growing trend in the fusion of biology and engineering. The ability to design and fabricate complex structures by printing living cells, biomaterials and other biological molecules is crucial to the success of tissue engineering^{1,2}, and is enabling new possibilities in drug screening and toxicology^{3,4}. In the continuing quest to engineer functional tissues and organs, bioprinting could allow the fabrication of multi-cellular constructs where cell-cell and cell-material interactions mimic the physiological environment and where cellular responses to stimuli are more reflective of those found *in vivo*.

The suite of bioprinting techniques that allow the controlled deposition of living cells has expanded to include extrusion printing^{5,6} and laser printing^{7,8}, as well as drop-on-demand approaches like microvalve printing^{9,10} and inkjet printing¹¹⁻¹⁴. Drop-on-demand techniques are attractive due to their relative simplicity and capability for precise non-contact deposition, yet have been hindered by some critical limitations. Cell settling and aggregation within printer reservoirs obstructs nozzles and leads to non-uniform cell distribution so that cell output significantly decreases or fails when printing over long time periods¹⁵. Gentle agitation of inkjet print heads and microvalves can reduce cell settling^{16,17} and addition of ethylenediaminetetraacetic acid limits aggregation¹⁸, but these strategies are only partly effective and can be detrimental to cell viability. Printing cells in high viscosity collagen solutions can retard settling, although this approach is limited to specialized printing systems⁹.

Inkjet printing presents additional challenges as the ink must meet stringent fluid property requirements (e.g. viscosity and surface tension) for efficient deposition¹⁹. Currently, non-ideal ink formulations have been printed using single- or few-nozzle

devices^{11,13,20,21}, or outdated thermal inkjet heads^{12,14,22-24}. Piezoelectric inkjet print-heads with multiple nozzles are the current standard for high-end printing applications, and could allow for higher throughput and fabrication of larger cellular constructs. Rather than developing bio-inks that are suitable for use in these systems, bio-ink design has focused on two-component fast-gelling reactive schemes. Cells have been mixed with alginate and printed into cross-linking Ca²⁺ solutions^{20,25}, or mixed with Ca²⁺ and printed into either alginate or alginate/collagen solutions²⁶. Similar approaches have utilized the fibrin/thrombin reaction^{22,23} or photo-polymerisable inks²⁴. However, these printed environments are not suitable for all cell types and applications. To deliver on the initial promise of drop-on-demand cell printing, we must develop smarter bio-inks that are tailored to satisfy the seemingly disparate demands of printability and cell function, and are amenable to printing using standard hardware.

Here, we report on the development of a general purpose bio-ink that addresses these challenges to allow facile cell deposition by drop-on-demand printing using both a commercial microvalve deposition system, and many-nozzle piezoelectric inkjet print heads.

Experimental

Bio-ink

Endotoxin-free low-acyl gellan gum (Gelzan CM, a gift from CP Kelco) was dissolved in hot (80°C) Milli-Q water (resistivity 18.2 MΩ cm) at 1% w/v by stirring for 1-2 hrs. This hot solution was combined with heated (80°C) Milli-Q and 2x concentrated Dulbecco's Modified Eagles Medium (DMEM, Invitrogen) to produce a range of gellan gum concentrations in 1x DMEM. The mixture was sheared using a vortex mixer while cooling to 25°C to create a microgel suspension, i.e. the bio-ink. The surfactant-

containing bio-inks were prepared through addition of Poloxamer 188 surfactant (Lutrol® F68, Sigma) and/or fluorosurfactant (Novec® FC-4430, 3M) solutions to the microgel suspension. All bio-inks were prepared under aseptic conditions.

5 Cell culture

C2C12 (CRL-1772), PC12 (CRL-1721) and L929 (CCL-1) murine cell lines were obtained from ATCC. C2C12 and L929 cells were maintained in DMEM (Invitrogen) supplemented with 10% fetal bovine serum (FBS, Invitrogen), while PC12 were maintained in DMEM with 10% fetal bovine serum and 5% horse serum (HS, Sigma). Cells were cultured at 37°C in a humidified incubator with 5% CO₂ and passaged every 2-3 days.

Bio-ink characterization

Rheology of the bio-ink was characterized using a controlled-stress ARG2 rheometer (TA Instruments), using a sandblasted 40 mm parallel plate geometry with a measurement gap of 0.5 mm and Peltier plate thermal control. A solvent trap was used to prevent evaporation of water during measurements. After loading, samples were subjected to 30 seconds pre-shear at 500 s⁻¹ followed by 1 min equilibration before measurement. Shear-dependent viscosity was measured by a stepped ramp of shear rate from 1-1000 s⁻¹. Each shear rate (10 points/decade) was held for 20 secs, and the viscosity over the last 10 secs was averaged. Apparent yield stress was measured by a continuous ramp of shear stress from 0-2 Pa over 5 min.

Constitutive modelling was facilitated by Rheology Advantage data analysis software (TA Instruments). Silicone oil standards (Scientific Polymer Products) were used to validate experimental conditions. Surface tension was measured using a Dataphysics OCA contact angle system with SCA 20 software.

The structure of the bio-ink was visualized by negative staining with a pigmented ink (Derivan Ink, black) that was excluded from microgel particles. Derivan Ink (1:5) was added to the bio-ink, 20 µL was immediately placed on a glass slide and cover-slipped prior to imaging.

The ability of the bio-ink to maintain cells in suspension was determined by suspending cells at 1-6x10⁶ cells/mL in the ink or in serum-free DMEM as the control. 100 µL aliquots of both suspensions were added to 96-well plates, and the base of each well was imaged over time. Image J software was used to count the number of cells in a defined area of the wells at each time-point, allowing the number of settled cells to be plotted as a function of time.

Printer design

Microvalve cell printing was facilitated through a Deerac™ GX1 liquid handling system (Labcyte Inc.), which dispenses droplets using a magnetic feedback-controlled microvalve. Cells were inkjet printed using a custom-built inkjet printing system with Xaar-126 piezoelectric inkjet print heads (Xaar®, see the Electronic Supporting Information). Both printers were housed in a bio-safety cabinet and sterilised regularly using 70% ethanol and UV light.

Cell printing.

For microvalve printing, C2C12 cells were suspended in the bio-ink (without added surfactants) at 2x10⁵-2x10⁶ cells/mL and

aspirated into the Deerac™ GX1 nozzle reservoir. Patterns were designed using accompanying software (Spot Station/Plate Designer). For analysis of cell viability and proliferation, 50 drops were printed into 100 µL of cell culture media supplemented with 100 units/mL penicillin and 100 µg/mL streptomycin (Pen/Strep, Gibco). For inkjet printing, cells (C2C12 or PC12) were suspended in the surfactant-containing bio-ink at 1-6x10⁶ cells/mL, and loaded into the print heads by aspirating through the nozzle plate. Patterns were designed in Microsoft Paint and loaded into Xaar XUSB software.

For analysis of cell viability, proliferation and differentiation, rectangular patterns (25x50 drops) were printed into supplemented media as above. This media was contained within thin (1 mm) PDMS wells (Fig. S2), and subsequently transferred to a 96-well plate for further culture and analysis.

For analysis of the cells/drop distribution, cells were printed directly onto glass slides and allowed to dry. The number of cells in each drop, or the number of cells in a printed pattern, was then counted manually or imaged using a Zeiss Axiovert 40 CFL inverted fluorescence microscope (Carl Zeiss AG) and counted using Image Pro software.

For patterning experiments, cells were inkjet printed onto collagen bio-paper. Collagen I (rat tail, 5 mg/mL, Invitrogen) was sonicated for 5 mins on ice, combined with cold 5x concentrated DMEM to a final concentration of 4 mg/mL and neutralised with 0.1M NaOH. The cold collagen solution was pipetted into 0.5 mm thick PDMS wells and polymerized for 2 hrs at 37°C. 1 mm thick PDMS wells were then placed on top of the existing PDMS to create a media reservoir (Fig. S2). Collagen bio-papers were rehydrated in cell culture media supplemented with Pen/Strep for 1-2 hrs, and excess media was removed prior to cell printing. Cell patterns were printed onto collagen bio-papers, and incubated at 37°C for 1 hr to allow cells to attach prior to further addition of culture media. In dual cell printing experiments, cells were stained prior to printing with CellTracker™ Probes (Molecular Probes, Invitrogen). C2C12 cells were stained with CellTracker™ Red CMPTX (20 µM) and PC12 cells were stained with CellTracker™ Green CMFDA (20 µM), following the manufacturers protocols.

Details on methods for cell viability, cell proliferation and differentiation and immunostaining can be found in the Electronic Supporting Information.

Results and Discussion

We prepared bio-inks by producing microgels (a dispersed phase of discrete polymeric gel particles) in standard cell culture media (Dulbecco's Modified Eagles Medium, DMEM) using the biopolymer gellan gum. This linear anionic polysaccharide has found widespread use in the food and cosmetic industries as a gelling and stabilizing agent²⁷, and more recently as a material for tissue engineering applications²⁸⁻³⁰.

The choice of use gellan gum over a more widely employed polysaccharide such as alginate is justified as follows. Gellan gum is a linear anionic polysaccharide similar to alginate³¹. The key difference between these two biopolymers is their gelation mechanism. Association of alginate chains during gelation occurs according to an 'egg-box' model³¹, where divalent cations bind pairs of polymer chains through the formation of stable junction

zones. In contrast, gelation of gellan gum is preceded by a conformational transition from coil to double helix, and association of these helices in junction zones is facilitated through either monovalent or divalent cations³². Consequently, gellan gum hydrogels may be formed at lower concentrations of divalent cations than those required for alginate. Gellan gum can even form gels in the presence of monovalent cations alone.

Gellan gum is particularly attractive for its ability to form microgels at low concentrations³³, which allows the mass content of the bio-ink to be kept at low levels. Furthermore, the concentration window to form microgels is much broader for gellan gum compared to that of alginate³⁴. A range of gellan gum concentrations was investigated and 0.05% w/v was the lowest concentration at which microgels form (Fig. S4). Imaging of the bio-ink structure at this concentration clearly revealed an associated network of elongated microgel particles (Fig. 1a). This tenuous network structure imparted pseudo-plastic properties that we elucidated by rheological measurements of both the apparent yield stress, and the apparent viscosity as a function of shear rate. The bio-ink exhibited an apparent yield stress of ~ 30 mPa (Fig. S3a) followed by shear-thinning flow behaviour that showed good agreement with constitutive modeling (Fig. S3b).

and cartoons depicting the ability of the microgel suspension to keep cells in suspension. (c) Average number of cells per drop over time, normalized to the number of cells in initial drops, for C2C12 cells suspended at 2×10^5 cells/mL in DMEM (open squares) or bio-ink (filled circles) and deposited by microvalve printing. Error bars represent one standard error of the mean ($n=10$). Statistically significant difference (compared to $t=0$ min) was assessed by unpaired Student's t -test and reported with 99% (**) or 99.9% confidence (***). (d) Spiral patterns of C2C12 cells suspended in bio-ink and deposited on a glass slide by microvalve printing. Scale bar 500 μ m.

Importantly, these properties are suitable to satisfy the dual aims of cell-suspending ability and printability. Cell settling in a fluid can be described by Stoke's law¹⁵, which defines a minimum yield stress of ~ 5 mPa for zero settling velocity. Thus the yield stress of the bio-ink is, theoretically, sufficient to keep cells suspended. Additionally, the shear-thinning behaviour presents a high viscosity to settling cells (shear rates <10 s⁻¹) to maintain suspensions, and a low viscosity during droplet ejection (shear rates $>10^3$ s⁻¹) to aid printability. To confirm this we performed cell settling tests and found that cells in the bio-ink remained suspended with no sign of aggregation, whereas cells suspended in DMEM alone completely settled to the base of a 96-well plate within 15 mins (Fig. 1b). The consequences of this for drop-on-demand cell printing were directly demonstrated by analyzing cell output over time by microvalve deposition. With DMEM

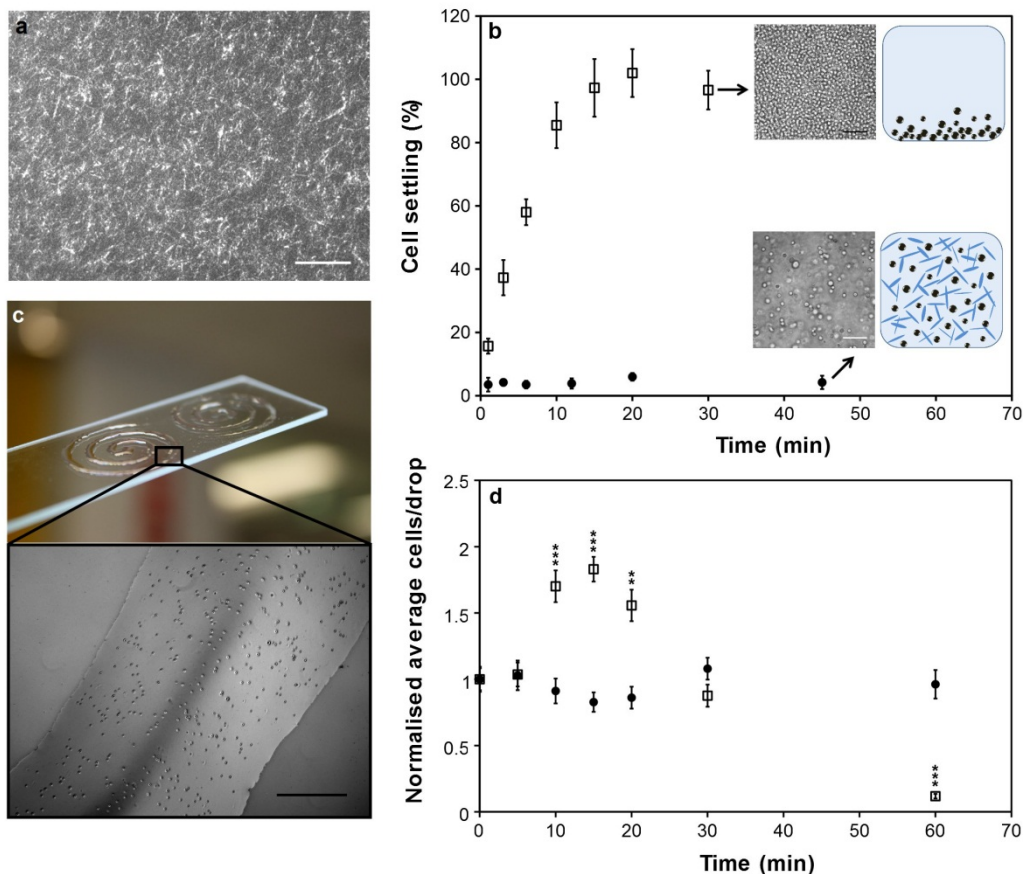



Fig. 1. Bio-ink structure and cell settling. (a) Structure of the bio-ink visualized by staining with Derivan ink and imaged by phase-contrast microscopy. Scale bar 200 μ m. (b) Cell settling (percentage of cells on the base of a 96 well plate) as a function of time for C2C12 cells suspended at 1×10^6 cells/mL in DMEM (open squares) or bio-ink (filled circles). Error bars represent one standard deviation from the mean. Insets show the base of well plates at indicated time points (scale bars 100 μ m)

alone, cell output showed significant variation with a sharp peak due to cell settling followed by a steady decrease during the deposition of cell-depleted media, whilst cell output was steady over 1 hour of printing with the bio-ink (Fig. 1c). This allowed the deposition of relatively large-scale patterns with uniform cell

distribution (Fig. 1d). Previous work has shown that printing cells from bio-inks consisting of cell culture media alone leads to inconsistent cell output from both microvalve¹⁷ and inkjet¹⁵ printing systems. This was attributed to cell settling and aggregation. Our bio-ink addresses these challenges to achieve consistent cell output.

Efficient deposition of the bio-ink by inkjet printing required the addition of surfactants that reduced the surface tension to the required low (~ 30 mN/m) levels without cytotoxicity. The non-ionic polymeric surfactant Poloxamer 188 (P188) is an established media additive which has been well-documented for protecting cells from fluid-mechanical damage³⁵. However, P188 alone did not sufficiently reduce the surface tension (Fig. S3c).

To achieve further surface tension reduction we investigated fluorinated surfactants, which exhibit both greater surface activity³⁶ and lower cytotoxicity³⁷ than their hydrocarbon analogues. We established that addition of 0.05% v/v of the non-ionic polymeric fluorosurfactant Novec FC-4430 in combination with 0.1% v/v P188 reduced the surface tension of the bio-ink to ~ 30 mN/m (Fig. S3c). To the best of our knowledge, this is the first example where surfactants have been utilised to achieve considerable surface tension reduction in a bio-ink, to within the optimal range for inkjet printing¹⁹ whilst maintaining the biocompatibility of the bio-ink. Importantly, this enabled controlled deposition of three different murine cell lines from commercially available Xaar-126 piezoelectric print heads. The use of these print heads represents a significant advance over currently employed piezoelectric print heads that have only a single nozzle^{13,20,21}. C2C12 (skeletal muscle), PC12 (neuronal model) and L929 (fibroblast) cells were reproducibly deposited from all 126 nozzles of the Xaar-126 print heads during numerous print cycles. Analysis of printed C2C12 patterns showed even cell density across the width of the print head (Fig. 2a-b), and by optimizing cell concentration in the bio-ink it was possible to print droplets that contained, on average, one cell per drop (Fig. 2c-d). The number of cells in each individual droplet followed the expected Poisson distribution (Fig. 2d), as previously observed by others using single-nozzle deposition methods^{21,38}.

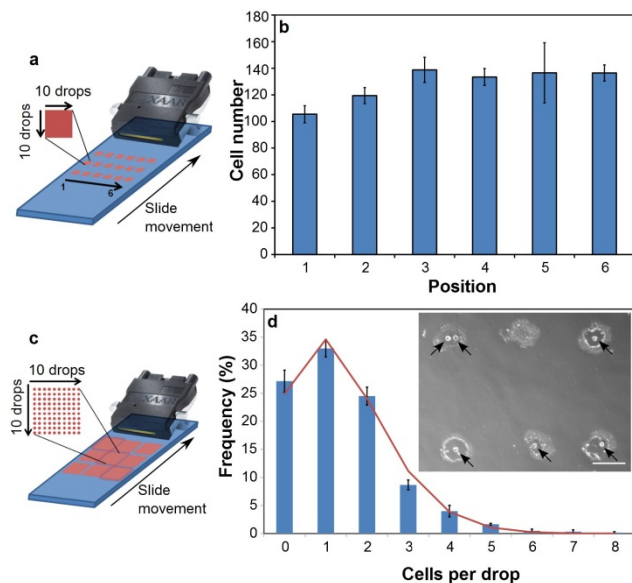

40

Fig. 2. Printing cells from one inkjet print head. (a) Printed cell number across print head width was analyzed by counting cells printed in squares of 10x10 droplets (utilizing 10 nozzles each). Each sample contained 18 replicate squares as illustrated, printed in a single pass. (b) Cell number in the six squares positioned across the print head width, averaged for the three vertical replicates in three samples printed sequentially. Error bars represent one standard error of the mean (n=3). One-way ANOVA indicated no statistically significant difference between the number of printed cells in each of the six positions. (c) Cells per drop distribution was analyzed by counting cells in individual drops printed in 10x10 arrays. Each sample contained 9 replicate arrays as illustrated, printed in a single pass. (d) Frequency distribution (bars) of the number of cells within individual printed droplets. Values were obtained by averaging the distributions in 3 arrays across the print head for two samples printed sequentially. Error bars represent one standard error of the mean (n=3). Line graph represents a Poisson distribution, calculated using the total average of cells per drop in the analysed arrays. Inset. Single printed droplets on glass containing C2C12 cells (black arrows). Scale bar 200 μ m.

Exposure to the bio-inks (with and without surfactants) did not have an apparent cytotoxic effect on either C2C12 or PC12 cells (Fig. 3a). In fact, the viability of bio-ink exposed PC12 cells was significantly higher than control cells exposed to DMEM alone. This is likely due to the maintenance of a single cell suspension in the bio-inks, as opposed to cells in DMEM which aggregated and settled and thus had to be re-suspended intermittently. Inkjet printed PC12 cells, and both inkjet and microvalve printed C2C12 cells, retained > 95% viability (Fig. 3a) and were shown to proliferate over 48 hrs at a rate comparable to non-printed controls (Fig. 3b).

A comparison of immunostained cells indicated that inkjet printed C2C12 and PC12 cells retained the ability to differentiate (Fig. 3c). Furthermore, removal of P188 from the surfactant-containing bio-ink decreased the viability of inkjet printed C2C12 cells (Fig. 3d), indicating a direct protective effect of P188 during the inkjet printing process. To demonstrate the utility of the surfactant-containing bio-ink to prevent cell settling during inkjet printing, we compared C2C12 cells printed immediately and then 1 hr after loading into the print head. After a 1 hr pause in printing, cell viability and density (average cells/drop) was no different to initial values (Fig. 3e). Representative images of live/dead stained cells printed at these different time points (Fig. 3e) show cells with similar density, morphology and viability. Taken together, these results establish the bio-inks as providing a unique combination of printability and cell-suspending capability whilst retaining the viability and function of printed cells.

Printing multiple cell types from different print heads is a highly attractive feature of inkjet printing as a biofabrication tool, allowing the fabrication of more complex multi-cellular constructs. Fig. 4a and 4b show two cell types (C2C12 and PC12) printed simultaneously from two different inkjet print heads in defined two-dimensional patterns onto collagen hydrogel substrates. Deposition of cells onto thin layers of collagen hydrogels ensured that the cells remained hydrated and viable for long enough to develop adhesions to the collagen, so that further addition of media did not disrupt the printed pattern. The cells were cultured under differentiation conditions and subsequently fixed and immunostained to assess the retention of printed patterns and the establishment of post-printing cell-cell and cell-substrate interactions. (The bio-ink did not impede cellular

100

interactions with the collagen substrate and both neural (PC12) and skeletal muscle (C2C12) cells were unimpeded in their ability to express the respective neural (β -III tubulin) and skeletal muscle (desmin) markers and to differentiate normally, as evidenced by the extension of dense neural networks from PC12 cells into surrounding areas populated by skeletal muscle cells (Fig. 4c and 4d).

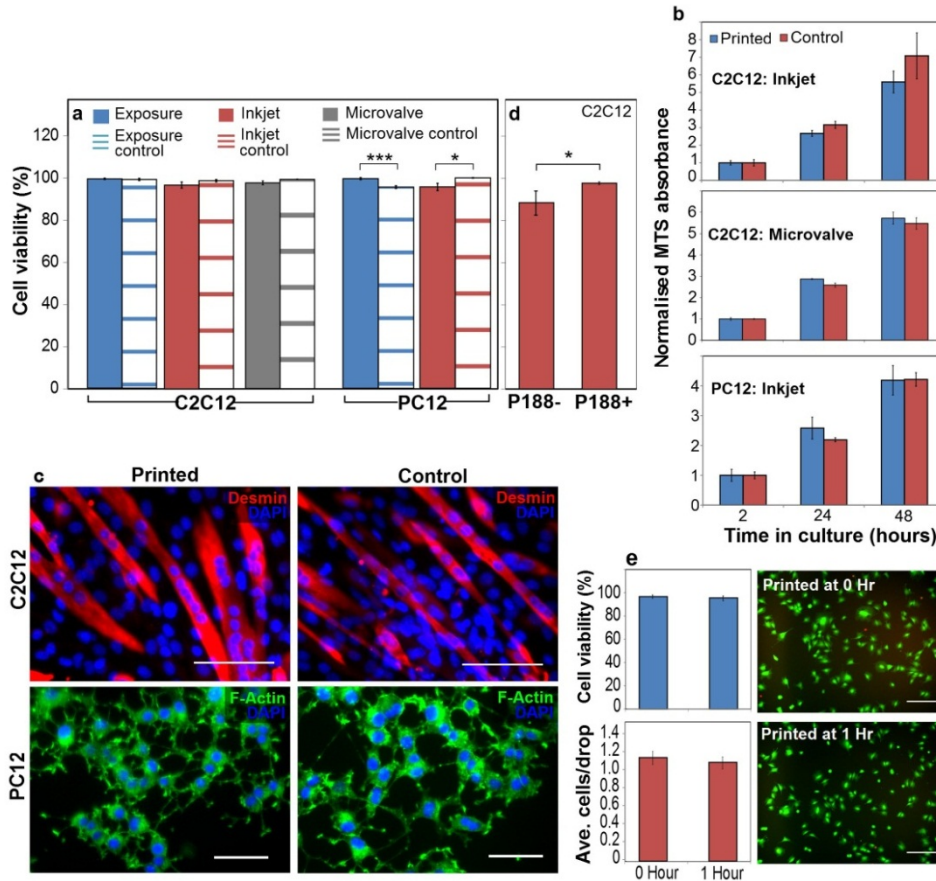


Fig. 3. Printed cell viability, proliferation and differentiation. (a) Viability (assessed by live/dead staining after 2 hrs in culture) of C2C12 and PC12 cells from typical experiments where cells were either suspended in the bio-ink for 2 hrs and pipetted into culture wells ('exposure' condition), or suspended in the bio-ink and printed into cell culture media by inkjet or microvalve printing. Control cells were suspended in DMEM for 2 hrs and pipetted into culture wells. (b) MTS assay indicating proliferation of printed C2C12 (microvalve and inkjet printed) and PC12 (inkjet printed) cells in comparison to non-printed controls over 48 hrs in culture. MTS absorbance was normalized to the 2 hour time point to account for differences in initial cell numbers. (c) Differentiated C2C12 and PC12 cells on tissue culture polystyrene, comparing inkjet printed and control cells. Cells were stained for desmin (C2C12) or F-actin (PC12) as described in Materials and Methods (scale bars 100 μ m for C2C12, or 50 μ m for PC12). (d) Viability (after 2 hrs in culture) of C2C12 cells printed from bio-ink containing 0.1% v/v P188 (P188+), or with this surfactant removed (P188-). (e) Comparison of C2C12 cells inkjet printed immediately and 1 hr after loading the cells into inkjet print head. Top left – printed cell viability at both time points assessed by live/dead staining after 2 hrs in culture. Bottom left – average number of cells/drop at both time points. Right – Representative live/dead images of cells at both time points (scale bars 200 μ m). (a, b, d, e) Error bars represent one standard error of the mean (n=3), and statistical significance was assessed by an unpaired Student's *t*-test and reported with either 99.9% (***) or 95% (*) confidence.

Conclusions

The results reported in this work demonstrate key advances towards addressing the major challenges in the continuing evolution of drop-on-demand cell printing towards becoming a clinically relevant biofabrication tool. Primarily, our bio-inks display optimal fluid properties whilst addressing the multiple complications that arise from cell settling and aggregation. As we have demonstrated, this means that cell-containing structures can be printed simultaneously from separate print heads, over extended time periods while maintaining printed cell density and viability. This capability is fundamental to the fabrication of multi-cellular and/or larger structures.

In this work even the printing of relatively simple dual-cell-type patterns in two dimensions was a time consuming task, and would not have been possible had the issues of cell settling and aggregation not been addressed. That printing was reproducible across the width of these print heads is further evidence of the utility of the bio-inks. It will allow more facile cell deposition,

and enhance the accessibility of the technique by enabling the use of standard commercially available print heads. This work shows that smarter designs of bio-ink formulations can lead to important advances in cell printing approaches.

5

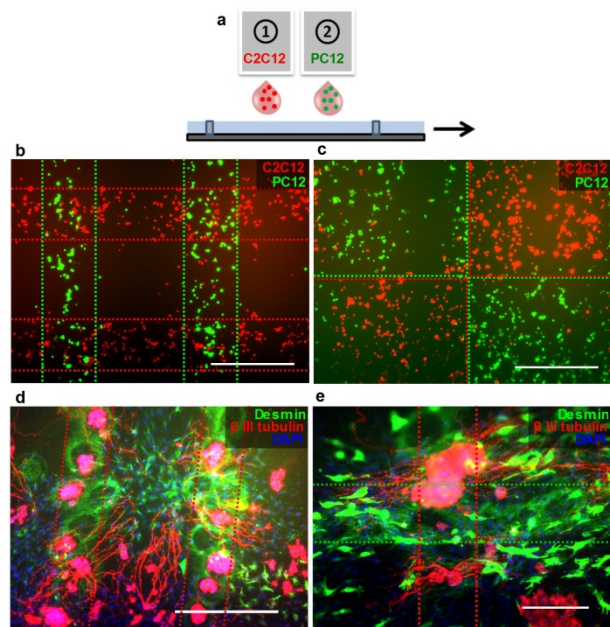


Fig. 4. Patterning of two cell types printed simultaneously from two separate inkjet print heads onto collagen substrates. (a) Schematic representation of multiple head printing. (b, c) C2C12 (red) and PC12 (green) cells pre-stained with CellTracker™ dyes and printed in various patterns. Images were taken 1 hr after printing, following the addition of culture media. (d, e) Printed patterns of C2C12 and PC12 cells after 8 days under differentiation conditions. Cells were immunostained for desmin (C2C12, green) and β-III tubulin (PC12, red). Dotted lines represent outline of printing pattern. Scale bars represent 500 μm (B-D) and 200 μm (E).

Acknowledgements

This work was supported by University of Wollongong (C.J.F.), and Centre of Excellence, Laureate (G.G.W.) and Future Fellowship (M.i.h.P.) funding from the Australian Research Council (ARC). We thank P. Jackson and R.C. Clark (both from C.P. Kelco) for provision of gellan gum and advice on rheology.

Notes and references

^a Intelligent Polymer Research Institute, ARC Centre of Excellence for Electromaterials Science, AIIIM Facility, University of Wollongong, Wollongong, NSW 2522, Australia. Tel: +61 24221 3155; E-mail: gwallace@uow.edu.au

^b Soft Materials Group, School of Chemistry, University of Wollongong, Wollongong, NSW 2522, Australia. Tel: +61 24221 3155; E-mail: panhuis@uow.edu.au

† Electronic Supplementary Information (ESI) available: diagram of inkjet printing, PDMS well, rheology and surface tension of bio-ink, and methods for cell viability, cell proliferation and differentiation and immunostaining. See DOI: 10.1039/b000000x/

1. P. Calvert, Printing cells, *Science* **318**, 208-209 (2007).

2. B. Guillotin, F. Guillemot, Cell patterning technologies for organotypic tissue fabrication, *Trends Biotechnol.* **29**, 183-190 (2011).

3. D. Castel, A. Pitaval, M. A. Debily, X. Gidrol, Cell microarrays in drug discovery, *Drug Discov. Today* **11**, 616-622 (2006).
4. M. L. Yarmush, K. R. King, Living-cell microarrays., *Annu. Rev. Biomed. Eng.* **11**, 235-257 (2009).
5. V. Mironov et al., Organ printing: tissue spheroids as building blocks, *Biomaterials* **30**, 2164-2174 (2009).
6. R. Gaetani et al., Cardiac tissue engineering using tissue printing technology and human cardiac progenitor cells, *Biomaterials* **33**, 1782-1790 (2012).
7. N. R. Schiele et al., Laser-based direct-write techniques for cell printing, *Biofabrication* **2**, 032001 (2010).
8. M. Gruene et al., Laser Printing of Stem Cells for Biofabrication of Scaffold-Free Autologous Grafts, *Tissue Eng. Pt-C. Meth.* **17**, 79-87 (2011).
9. S. J. Moon et al., Layer by layer three-dimensional tissue epitaxy by cell-laden hydrogel droplets, *Tissue Eng. Pt-C. Meth.* **16**, 157-166 (2010).
10. F. Xu et al., A droplet-based building block approach for bladder smooth muscle cell (SMC) proliferation, *Biofabrication* **2**, 014105 (2010).
11. W. C. Wilson, T. Boland, Cell and organ printing 1: protein and cell printers, *Anat. Rec. Part A* **272**, 491-496 (2003).
12. T. Xu, J. Jin, C. Gregory, J. J. J. Hickman, T. Boland, Inkjet printing of viable mammalian cells, *Biomaterials* **26**, 93-99 (2005).
13. R. E. Saunders, J. E. Gough, B. Derby, Delivery of human fibroblast cells by piezoelectric drop-on-demand inkjet printing, *Biomaterials* **29**, 193-203 (2008).
14. T. C. Burg, C. a P. Cass, R. Groff, M. E. Pepper, K. J. L. Burg, Building off-the-shelf tissue-engineered composites, *Philos. T. R. Soc A* **368**, 1839-1862 (2010).
15. M. E. Pepper, V. Seshadri, T. C. Burg, K. J. L. Burg, R. E. Groff, Characterizing the effects of cell settling on bioprinter output, *Biofabrication* **4**, 011001 (2012).
16. S. Parsa, M. Gupta, F. Loizeau, K. C. Cheung, Effects of surfactant and gentle agitation on inkjet dispensing of living cells, *Biofabrication* **2**, 025003 (2010).
17. W. Lee et al., Multi-layered culture of human skin fibroblasts and keratinocytes through three-dimensional freeform fabrication, *Biomaterials* **30**, 1587-95 (2009).
18. C. A. Parzel, M. E. Pepper, T. C. Burg, R. E. Groff, K. J. L. Burg, EDTA enhances high-throughput two-dimensional bioprinting by inhibiting salt scaling and cell aggregation at the nozzle surface, *J. Tissue Eng. Regen. M.* **3**, 260-268 (2009).
19. B. Derby, Inkjet Printing of Functional and Structural Materials: Fluid Property Requirements, Feature Stability, and Resolution, *Ann. Rev. Mater. Res.* **40**, 395-414 (2010).
20. K. Arai et al., Three-dimensional inkjet biofabrication based on designed images, *Biofabrication* **3**, 034113 (2011).
21. A. R. Liberski, J. T. Delaney, U. S. Schubert, "One cell-one well": a new approach to inkjet printing single cell microarrays, *ACS Combin. Sci.* **13**, 190-195 (2011).
22. T. Xu et al., Viability and electrophysiology of neural cell structures generated by the inkjet printing method., *Biomaterials* **27**, 3580-3588 (2006).
23. X. Cui, T. Boland, Human microvasculature fabrication using thermal inkjet printing technology, *Biomaterials* **30**, 6221-6227 (2009).
24. X. Cui, K. Breitenkamp, M. G. Finn, M. Lotz, D. D. D'Lima, Direct Human Cartilage Repair Using Three-Dimensional Bioprinting Technology., *Tissue Eng. Pt. A* (available at <http://www.ncbi.nlm.nih.gov/pubmed/22394017>).
25. Y. Nishiyama et al., Development of a three-dimensional bioprinter: construction of cell supporting structures using hydrogel and state-of-the-art inkjet technology, *J. Biomech. Eng.- T. ASME* **131**, 035001 (2009).
26. T. Xu et al., Characterization of Cell Constructs Generated With Inkjet Printing Technology Using In Vivo Magnetic Resonance Imaging, *J. Manuf. Sci. E.- T. ASME* **130**, 021013 (2008).
27. A. M. Fialho et al., Occurrence, production, and applications of gellan: current state and perspectives, *Appl. Microbiol. Biot.* **79**, 889-900 (2008).

-
28. A. M. Smith, R. M. Shelton, Y. Perrie, J. J. Harris, An initial evaluation of gellan gum as a material for tissue engineering applications, *J. Biomater. Appl.* **22**, 241-254 (2007).
29. C. J. Ferris, M. in het Panhuis, Conducting bio-materials based on gellan gum hydrogels, *Soft Matter* **5**, 3430-3435 (2009).
- 5 30. J. T. Oliveira et al., Gellan gum: A new biomaterial for cartilage tissue engineering applications, *J. Biomed. Mater. Res. A* **93A**, 852-863 (2010).
31. K. Y. Lee, D. J. Mooney, Alginate: properties and biomedical applications, *Prog. Polym. Sci.* **37**, 106-126 (2012).
- 10 32. E. R. Morris, K. Nishinari, M. Rinaudo, Gelation of gellan gum – a review, *Food Hydrocolloids* **28**, 373-411 (2012)
33. M. Caggioni, P. T. Spicer, D. L. Blair, S. E. Lindberg, D. A. Weitz, Rheology and microrheology of a microstructured fluid: The gellan gum case, *J. Rheol.* **51**, 851 (2007).
- 15 34. G. S. Sworn, G. R. Sanderson and W. Gibson, Gellan gum fluid gels, *Food Hydrocolloids* **9**, 265-271 (1995)
35. E. T. Papoutsakis, Media additives for protecting freely suspended animal cells against agitation and aeration damage, *Trends Biotechnol.* **9**, 316-324 (1991).
- 20 36. M. Krafft, Fluorocarbons and fluorinated amphiphiles in drug delivery and biomedical research, *Adv. Drug Deliver. Rev.* **47**, 209-228 (2001).
37. X. Li et al., Hydrophobic tail length, degree of fluorination and headgroup stereochemistry are determinants of the biocompatibility of (fluorinated) carbohydrate surfactants., *Colloid Surface B* **73**, 65-74 (2009).
- 25 38. J. A. Barron, D. B. Krizman, B. R. Ringeisen, Laser Printing of Single Cells: Statistical Analysis, Cell Viability, and Stress, *Ann. Biomed. Eng.* **33**, 121-130 (2005).
- 30